Megazyme Building 1,
Bray Business Park,
Bray, Co. Wicklow,
A98 YV29,
Ireland.
Tel: + 353 1 2861220 Fax: + 353 1 2861264

# Certificate of Analysis

**Product:** Laminaribiose
**Cat. No:** O-LAM2
**Lot. No:** 230402A
**Expiry Date:** N/A

**Parameters:**

| Purity By | Specification | Result |
|---|---|---|
| HPLC | >95% | 95.7% |

This lot meets our specification.

**Signature:** Ciara McLoughlin **Date:** 21.Apr.2023

Ciara McLoughlin

QC Manager

(*as this certificate is a computer printout, it has not been signed or dated by hand*)

© 2023, Neogen Corporation; © 2023, Megazyme. All rights reserved.
Neogen is a registered trademark of Neogen Corporation. Megazyme is a registered trademark of Megazyme Ltd.


Megazyme Building 1,
Bray Business Park,
Bray, Co. Wicklow,
A98 YV29,
Ireland.
Tel: + 353 1 2861220 Fax: + 353 1 2861264

**HPLC:**

Product: O-LAM2, Lot 230402A

Column: Shodex Asahipak NH2P-40 3E analytical column
Temperature: 35°C
Flow rate: 0.35 mL/min (Eluent gradient shown below)
Detector: CAD (Charged Aerosol Detector)
HPLC System: Thermofisher U3000 Ultimate and Chromeleon v 7.0 software

| Time (min) | $H_2O$ (%) | $CH_3CN$ (%) |
|---|---|---|
| 0 | 40 | 60 |
| 1 | 40 | 60 |
| 14 | 60 | 40 |
| 16 | 40 | 60 |
| 18 | 40 | 60 |
| 20 | 40 | 60 |

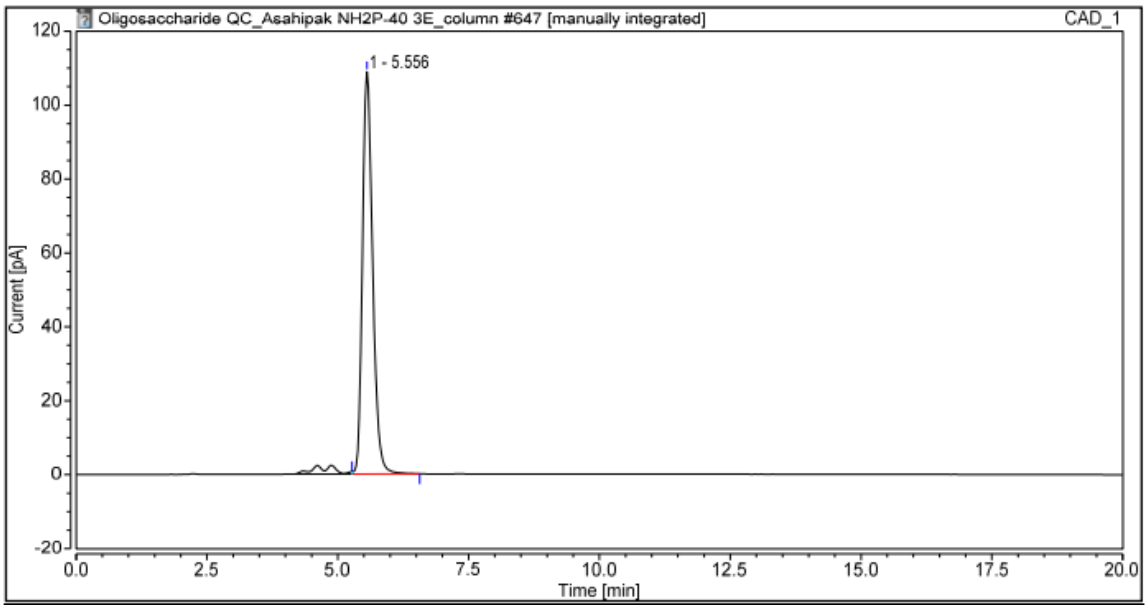


© 2023, Neogen Corporation; © 2023, Megazyme. All rights reserved.
Neogen is a registered trademark of Neogen Corporation. Megazyme is a registered trademark of Megazyme Ltd.